

PATIENT: XXXXXXXXXXXXXXXXXX

TEST NUMBER: T-NL-XXXXX (XXXXXXXXXXX)

GENDER: XYZ COLLECTED: XX/XX/XXXX RECEIVED: XX/XX/XXXX TESTED: XX/XX/XXXX

XXXXXXXXXXXX

TEST REF: TST-NL-XXXX

XXXXXXXXXXXXXXXXXXXX

TEST NAME: Breath Test for Sucrose Malabsorption/Intolerance


Summary Report of Hydrogen & Methane Breath Analysis with Carbon Dioxide Correction

Sample Normalization ¹					
ppm CO2	fCO2				
4.4	1.25				

Gasses Analyzed	Patient Result	Expected	
Increase in Hydrogen (H ₂)	38 ppm (high)	< 20 ppm	
Increase in Methane (CH ₄)	6 ppm (normal)	< 12 ppm	
Increase in combined H ₂ & CH ₄	44 ppm (high)	< 15 ppm ³	

Analysis of the data suggests	Sucrose intolerance is suspected ^{3,7}
-------------------------------	---

Number	Collection Interval	ppm H2	ppm CH4	Combined	ppm CO2	fCO2
1	Baseline	5	0	5	4.4	1.25
2	30 Min.	22	4	26	4.5	1.22
3	60 Min.	15	2	17	4.6	1.19
4	90 Min.	22	4	26	4.2	1.30
5	120 Min.	22	4	26	4.7	1.17
6	150 Min.	35	4	39	3.9	1.41
7	180 Min.	43	6	49	4.3	1.27

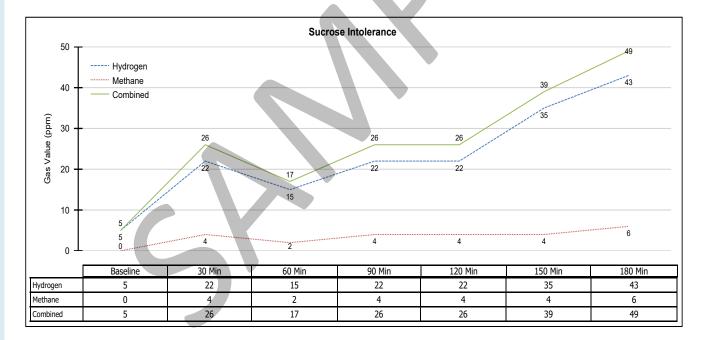

Important Information - Please Read:

Breath analysis standards for abnormal tests are suggested if an increase of 20ppm for Hydrogen (H2), 12ppm for Methane (CH4), or a combined 15ppm for Hydrogen (H2) & Methane (CH4) is detected.

Only the treating clinician is able to determine if there are additional factors that could have a material impact on the results of this analysis. A diagnosis can only be obtained from a medical professional that combines clinical information with the results of this breath analysis.

The results of this Hydrogen (H2) & Methane (CH4) breath test should be utilized as a guideline only.

Aerodiagnostics LLC does not have access to patient clinical information that is critical for a diagnosis determination

Quality Control:

Aerodiagnostics performs quality control analysis on specimens processed using rigorous standard operating procedures, established in conjuction with Clinical Laboratory Improvement Amendments (CLIA). Hydrogen (H₂) & Methane (CH₄) breath test values are corrected by Aerodiagnostics state-of-the-art solid state sensor technology & scientific algorithm for Carbon Dioxide (CO₂) content in the samples

1 The correction factor, f(CO2) is used to determine if each sample is valid for analysis. A f(CO2) close to 1.00 is indicative of a good alveolar sample, while a factor in excess of 4.00 is indicative of a poor sample ³ A combined H₂ + CH₄ increase of 15 ppm or more may be suggestive of Sucrose intolerance.

Elevated H2 and/or CH4 levels >120 minutes can indicate intolerance. Metz, G. et al. Breath hydrogen as a diagnostic... Lancet 1975 (May 24); 1(7917):1155-7. If the baseline H2 level is elevated and the onehour sample is elevated even more, there is a strong suspicion that the patient has bacterial overgrowth. Even with overgrowth, a later increase in H2 and/or CH4 can be interpreted as a positive test for intolerance. Douwes, AC, Schaap, C and van der Kleivan Moorsel, JM. Hydrogen breath test in school children. Arch Dis Child. 1985 (Apr);60(4):333-7

Nordic Laboratories Aps

Nygade 6, 3.sal • 1164 Copenhagen K • Denmark Tlf. +45 33 75 10 00

UK Office:

11 Old Factory Buildings • Stonegate • E. Sussex TN5 7DU • UK Tel: +44 (0)1580 201 687

Page 1 of 1 www.nordic-labs.com info@nordic-labs.com